

Information Data Sheet

Detector Tube Ethanol-100

Part No. (US): 804136

Part No. D5086818

1. Application

Detection of ethanol (ethyl alcohol, C₂H₅OH).

2. Detector Tube Sampling Pump

KWIK DRAW (formerly MSA AUER) Gas-Tester[®] IIH, Gas-Tester[®] I / ThumbPump[™]-Sampler, Toximeter[®] II, Uniphos Kwik-Draw[™]-Pump or other suitable detector tubes pumps. Observe respective instructions for use.


3. Measuring Range

100 ppm ... 3,000 ppm ethanol at n=10 (10 pump strokes).

4. Chemical Reaction and Color Change

Oxidation of ethanol by a chromate/sulfuric acid reagent.

Color change: Red → Greyish-green

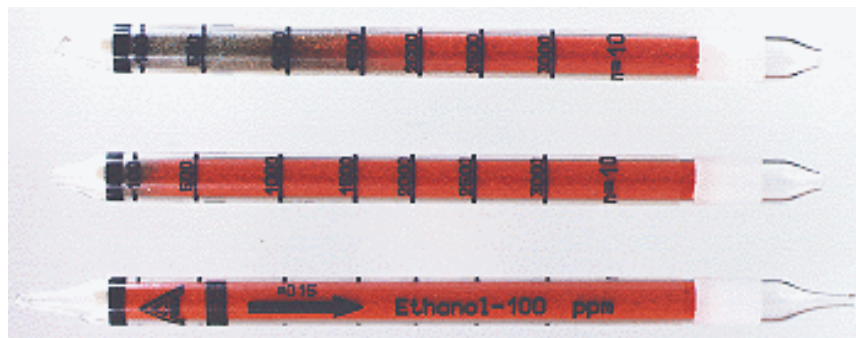

5. Ambient Conditions During Sampling

Detector tubes can be used without compensation of the reading between 0 °C and 30 °C (32 °F and 86 °F) and between 10% RH [0.5 g/m³ at 0 °C (32 °F)] and 90% RH [27 g/m³ at 30 °C (86 °F)].

6. Interferences and Cross Sensitivities

a) No interference from:

- hydrogen, hydrocarbons (methane, ethane, ethylene), carbon monoxide, carbon dioxide.
- halogenated hydrocarbons (e.g. trichloroethane, trichloroethyle, chlorobenzene), hydrogen sulfide, carbon disulfide, acetic acid up to 5,000 ppm.
- Aldehydes, ketones, ethers, esters up to 1,000 ppm.

Manufactured By:

Uniphos Envirotronic Pvt. Ltd (100% EOU)

P.O. Nahuli - 396 108

Tal. Umbergaon,

Dist: Valsad, Gujarat, India

Tel. : +91(260) 2730156 / 57 / 58

Fax : +91(260) 2730160

Marketing Office:

Uniphos Envirotronic Pvt. Ltd

Readymoney Terrace, 167,

Dr. Annie Besant Road, Worli,

Mumbai 400 018, India.

Tel. : +91(22) 6123 3500

Fax : +91(22) 2493 8826

+91 (22) 2497 8119