

Information Data Sheet

Detector Tube NH₃-20

Part No. (US): 800300

Part No. D5085814

1. Application

Detection of ammonia (NH₃) in air or in technical gases.

2. Detector Tube Sampling Pump

UNIPHOS KWIK DRAW (formerly MSA AUER) Gas-Tester[®] IIH, Gas-Tester[®] I / ThumbPump[™]-Sampler, Toximeter[®] II, Uniphos Kwik-Draw[™]-Pump or other suitable detector tubes pumps. Observe respective instructions for use.


3. Measuring Range

(20 ... 1,400) ppm ammonia at n=1 (1 stroke).

4. Chemical Reaction and Color Change

Change of pH-value causes color change of an acid-base-indicator.

Color change: yellow → blue.

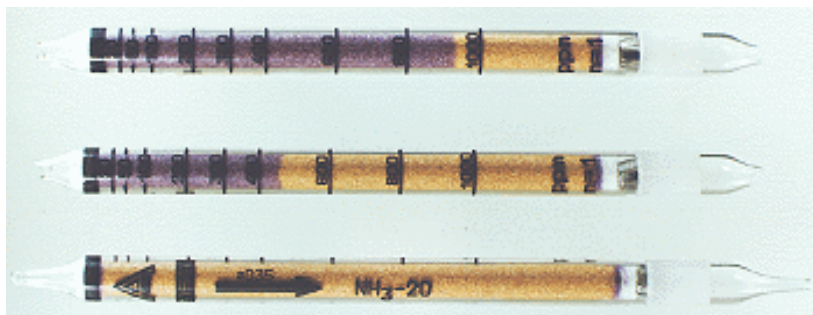

5. Ambient Conditions During Sampling

Detector tubes can be used without compensation of the reading between 10 °C and 30 °C (50 °F and 86 °F) and between 20% rh [1.9 g/m³ at 10 °C (50 °F)] and 80% rh [24 g/m³ at 30 °C (86 °F)].

6. Interferences and Cross Sensitivities

- a) No interference from:
 - carbon dioxide up to 4 vol %.
 - higher saturated hydrocarbons (e.g. hexanes, octanes), olefinic hydrocarbons (e.g. ethylene), aromatic hydrocarbons (e.g. benzene) up to 1 vol %.
 - hydrogen sulfide, nitrogen dioxide up to 1,000 ppm.
- b) Other alkaline gases (amins, hydrazine) will be indicated. The sensitivity of indication is different.
- c) Strong acidic gases (e.g. sulfur dioxide, hydrogen chloride, chlorine, phosgene) are not indicated but will shorten stain length of ammonia even when concentrations correspond to measuring range of detector tube.

Manufactured By:

Uniphos Envirotronic Pvt. Ltd

P.O. Nahuli - 396 108

Tal. Umbergaon,

Dist: Valsad, Gujarat, India

Tel. : +91(260) 2730156 / 57 / 58

Fax : +91(260) 2730160

gasdetection@uniphos.com

Marketing Office:

Uniphos Envirotronic Pvt. Ltd

Readymoney Terrace, 167,

Dr. Annie Besant Road, Worli,

Mumbai 400 018, India.

Tel. : +91(22) 6123 3500

Fax : +91(22) 2493 8826

+91 (22) 2497 8119

www.kwikdrawtubes.com