

Information Data Sheet

Detector Tube Triethylamine-5

Part No. (US): 804134

Part No. D5086816

1. Application

Detection of triethylamine ($N(C_2H_5)_3$).

2. Detector Tube Sampling Pump


KWIK DRAW(formerly MSA AUER) Gas-Tester[®] IIH, Gas-Tester[®] I / ThumbPump[™]-Sampler, Toximeter[®] II, Uniphos Kwik-Draw[™]-Pump or other suitable detector tubes pumps. Observe respective instructions for use.

3. Measuring Range

5 ppm ... 30 ppm triethylamine at n=1 (1 pump stroke).

4. Chemical Reaction and Color Change

Change of pH-value causes color change of an acid-base-indicator.
Color change: pink or yellow → green or blue.

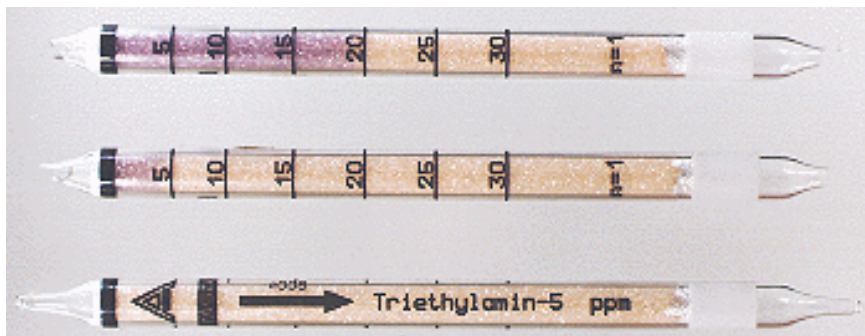

5. Ambient Conditions During Sampling

Detector tubes can be used between 10 °C and 30 °C (50 °F and 86 °F) and in the humidity range between 5 g/m³ (50 % RH at 10 °C [50 °F], 30 % RH at 20 °C [68 °F], 15 % RH at 30 °C [86 °F]) and 12 g/m³ (70 % RH at 20 °C [68 °F], 40 % RH at 30 °C [86 °F]).

6. Interferences and Cross Sensitivities

- No interference from:
 - Hydrogen, methane, ethane, propane, carbon monoxide.
 - Carbon dioxide up to 1 Vol. %.
 - Nitrogen dioxide, hydrogen sulfide up to 50 ppm.
- Ammonia and other alkaline gases and vapours (e.g. hydrazine) will be indicated. The sensitivity of indication is different.
- Strong acid gases (e.g. sulfur dioxide, hydrogen chloride) are not indicated but will decrease stain length of triethylamine indication even when concentrations correspond to measuring range of detector tube.

Manufactured By:

Uniphos Envirotronic Pvt. Ltd (100% EOU)

P.O. Nahuli - 396 108

Tal. Umbergaon,

Dist: Valsad, Gujarat, India

Tel. : +91(260) 2730156 / 57 / 58

Fax : +91(260) 2730160

Marketing Office:

Uniphos Envirotronic Pvt. Ltd

Readymoney Terrace, 167,

Dr. Annie Besant Road, Worli,

Mumbai 400 018, India.

Tel. : +91(22) 6123 3500

Fax : +91(22) 2493 8826

+91 (22) 2497 8119